



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser Micron Test Report

05/04/06

Test No: 273821


Animal and Sample Description

Animal Name: Skye
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: XXXXX
Sample Location: Side (L)
Sample Date: 04/19/06
Age: 12/22/05

Laboratory Data

Mean Fiber Diameter:	20.1 microns	Mean Staple Length:	72.0 mm
Standard Deviation:	4.4 microns	Length Standard Deviation:	4.2 mm
Coefficient of Variation:	22.0 %	Length Coefficient of Variation:	5.9 %
Spin Fineness:	19.8 microns	Mean Curvature:	34.3 deg/mm
Fibers Greater Than 30 microns:	2.1 %	SD Curvature:	23.1 deg/mm
Medullated Fibers:	8.4 %		

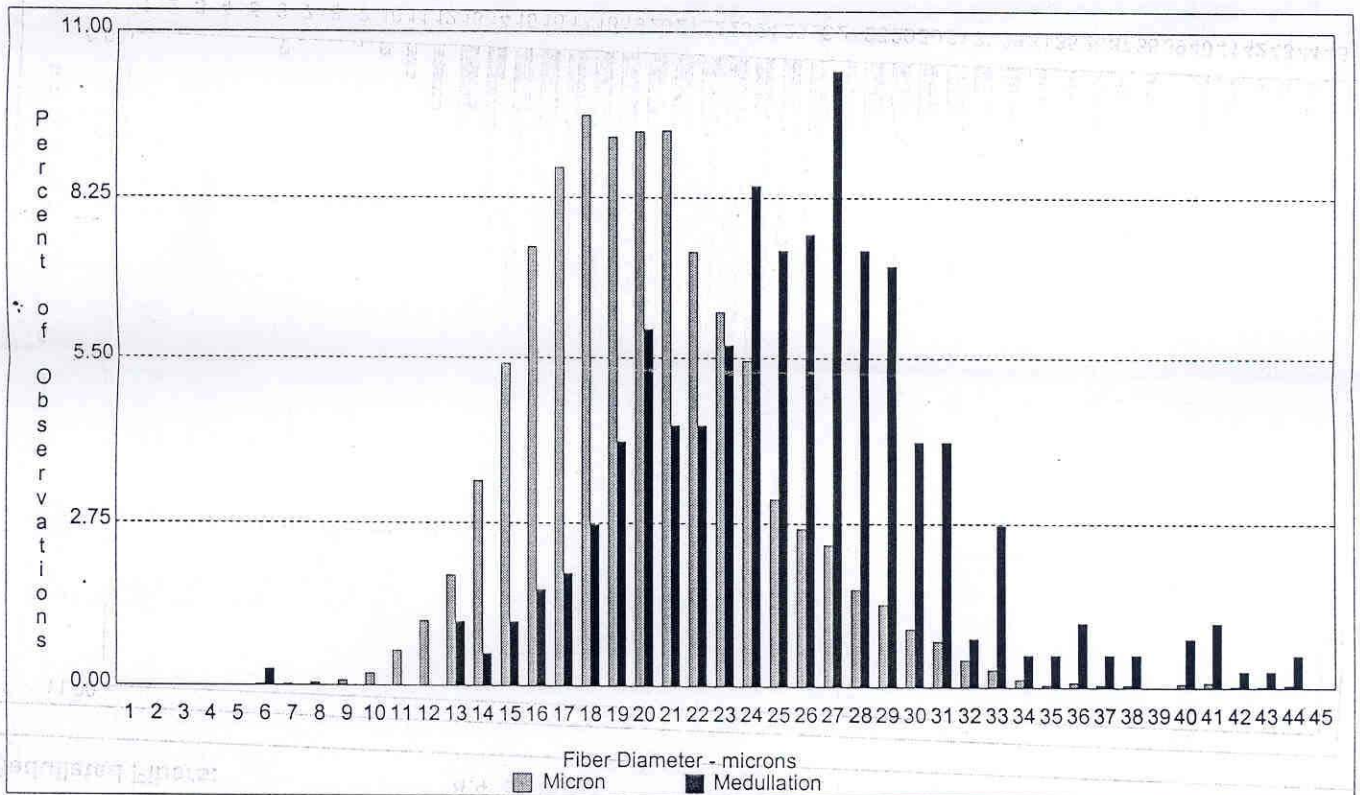

This Test Performed According to I.W.T.O Method 47